

In Vivo Three-Dimensional Kinematics of the Human Knee

Shojiro TERASHIMA*, Yoshinori ISHII**, Kazuhiro TERAJIMA***,
And Yoshio KOGA****

(Received October 30, 1997)

Knee motion was measured with an instrumented spatial linkage (accuracy ; linear $\pm 500 \mu\text{m}$, angular $\pm 0.5^\circ$) fixed with intracortical Kirschner wires in five healthy male volunteers (five knees, judged clinically to be normal). This technique allows an accurate description of the relative angular and linear movements between tibia and femur without the effect of skin movement relative to the bone, and changing muscle volume. Motion of the tibia relative to the femur was described in terms of three clinically meaningful rotations and three translations between full extension and 60° flexion: (a) abduction and adduction: $3.4 \pm 1.2^\circ$, (b) internal and external rotation: $10.6 \pm 2.8^\circ$; representing screw home motion, (c) anterior and posterior: $5.2 \pm 1.7 \text{ mm}$; representing roll back phenomenon, (d) proximal and distal: $1.2 \pm 2.7 \text{ mm}$, (e) medial and lateral: $1.1 \pm 2.6 \text{ mm}$.

Key words : Motion Analysis, In Vivo, Knee Kinematics, Three Dimensional

1. INTRODUCTION

Measurement of relative motion between the tibia and femur in vivo usually is accomplished indirectly, by attaching transducers to the soft tissues surrounding the calf and thigh. Skin movement relative to bone and change in muscle volume can influence these measurements. Thus, the precision of three-dimensional measurement of tibiofemoral motion has been limited because of the error introduced by the nonstationary soft tissues in both commonly used methods of goniometric^{8, 9, 13, 14, 22, 24, 25, 29, 32} and photogrammetric^{1, 2, 3, 4, 12, 18, 26} techniques. In an in vitro study, it is difficult to reproduce proper tension to muscles and ligaments that regulate knee motion and geometry. Therefore, there is still considerable question as to what constitutes normal motion at the knee.

The purpose of this study is to provide an accurate description of the relative angular and linear movements between tibia and femur without the effect of soft tissues, for knee flexion and extension, by in vivo use of an instrumented spatial linkage fixed with intracortical Kirschner wires (K wires).

*Department of Mechanical and Control Engineering, Research Associate

**Department of Orthopaedic Surgery, School of Medicine, Niigata Univ., Japan

***Department of Mechanical Engineering, Niigata Univ., Japan

****Niigata Kobari Hospital, Japan

2. MATERIALS AND METHODS

Five healthy male volunteers (five knees), with knees judged clinically to be normal, participated in this study. The subjects had a mean age of 26 ± 1 years, mean height of 170 ± 3 cm, and mean body weight of 63 ± 3 kg. Before the experiment began, the subjects signed a consent form that included an explanation of the procedures, a description of the experimental protocol, and potential for complication such as infection, discomfort, pain, pin related failures. This procedure was performed with the same infection control procedures as standard during operative procedures in surgical suites. Two K wires (2.4 mm diameter) were inserted with an electric orthopaedic drill into cortices of the left femur and tibia of the five subjects. The pins penetrated the bones in a medial direction from lateral, parallel to each other. The pin insertion sites were anesthetized with injections of 1% mepivacaine into surrounding soft tissues and periosteum. Before insertion of the pins into the bones, 5 mm width transverse incisions were made through the skin and soft tissues to prevent these structures from applying forces to the wires.

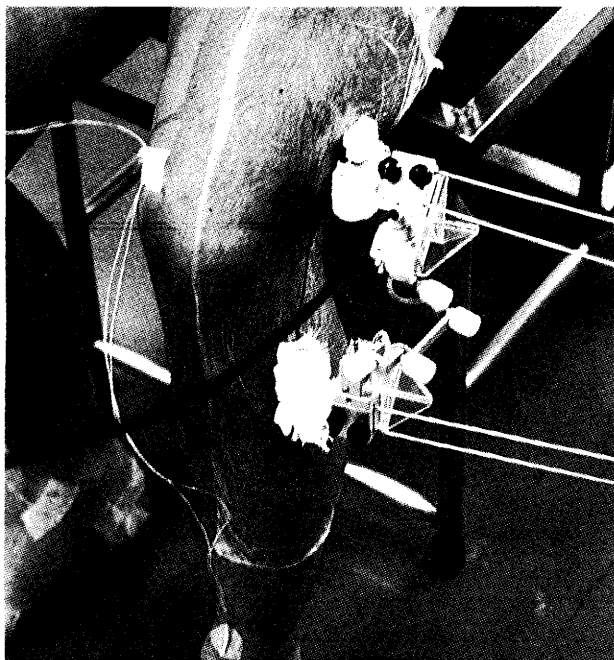


Figure 1: An instrumented spatial linkage fixed with intracortical Kirschner wires. Active knee motion between full extension and 60° flexion was analyzed while the subject was seated.

Knee joint kinematics were measured with a 6 degree of freedom instrumented spatial linkage attached to the K wires. The instrumented spatial linkage is composed of seven metal pieces or links interconnected by six electrical hinges or potentiometers. The ends of the instrumented spatial linkage are fixed to the tibia and femur so that the instrumented spatial linkage spans the joint. The links and potentiometers freely change their relative positions and orientations as the knee moves. By knowing the geometry of the links, the electrical parameters which characterize the potentiometer, and voltages generated by the potentiometers as the knee moves, the position of one end of the instrumented spatial linkage can be computed relative to the other end (Fig 1).

In Vivo Three-Dimensional Kinematics of the Human Knee

The linear accuracy of the instrumented spatial linkage was determined by placing the instrumented spatial linkage in known configurations on a milling machine, and comparing the known and predicted relative positions of the ends of the instrumented spatial linkage. The linear accuracy was determined to be $\pm 500 \mu\text{m}$, and the angular accuracy was $\pm 0.5^\circ$.³¹ Active knee motion between full extension and 60° flexion was analyzed while the subject was seated. (Sixty degrees flexion was chosen because it is thought to be the peak flexion angle in swing phase during normal gait and in the authors' gait analysis using the same instrumented spatial linkage²⁹). Also, limiting motion to 60° flexion avoided any pain to subjects. Average kinematic patterns of the tibia with respect to the femur were obtained from three trials in each of five subjects.

Motion between the ends of the instrumented spatial linkage was related to the anatomy of the knee through the application of a biplanar radiographic technique with the knee in full extension, to accurately calculate the dimensions of the femur and tibia (Fuji Computed Radiographic System, Fuji Film Inc, Tokyo, Japan) (Fig 2). Using the radiographic images of the knee joint and the targets on the ends of the instrumented spatial linkage, anatomic rotation axis directions were determined, and a point from which tibial translations would be defined. The origin of the femur was defined as the center of both condyles, and the origin of the tibia was defined as the center of the tibia plateau.^{28,30}



Figure 2: To transfer the instrumented spatial linkage's coordinate to the femur and tibia, biplanar X-rays were taken with the knee at full extension.

Motion of the tibia relative to the femur was described in terms of three clinically meaningful rotations (flexion and extension, internal and external rotation, abduction and adduction) and three translations (anterior and posterior, medial and lateral, proximal and distal). The calibration was performed on the system before and after each test and exhibited 0.5° in angular accuracy and $500\mu\text{m}$ in linear accuracy.

3. RESULTS

All subjects tolerated the protocol well. Knee kinematic data are shown in Figure 3. Motion of the tibia relative to the femur (average ± 1 standard deviation) was described in terms of three clinically meaningful rotations and three translations between full extension and 60° flexion : (a) abduction and adduction: $3.4 \pm 1.2^\circ$, (b) internal and external rotation: $10.6 \pm 2.8^\circ$; representing screw home motion, (c) anterior and posterior: $5.2 \pm 1.7\text{ mm}$; representing roll back phenomenon, (d) proximal and distal: $1.2 \pm 2.7\text{ mm}$, (e) medial and lateral: $1.1 \pm 2.6\text{ mm}$.

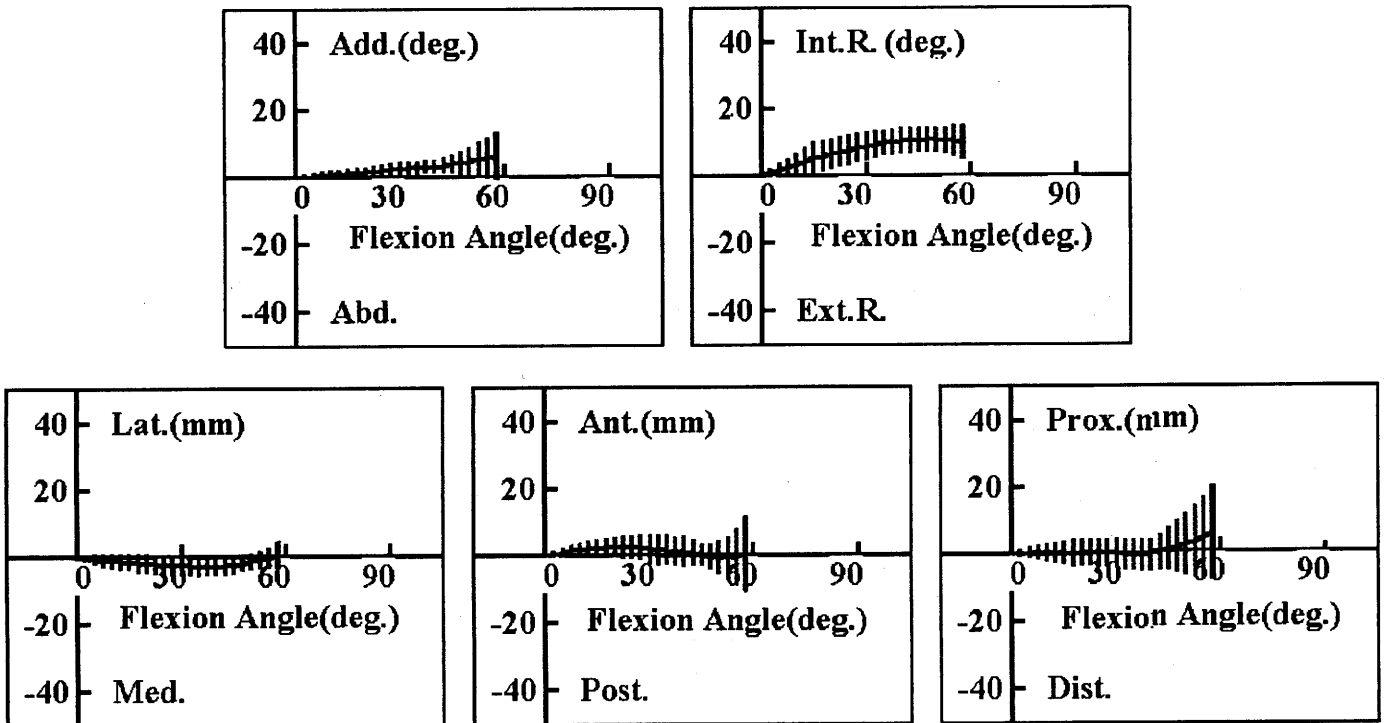


Figure 3: Average (Solid lines) and standard deviation (vertical bars) of angular and linear displacement of tibiofemoral joint between 60° flexion and extension at sitting position.

4. DISCUSSION

Although there have been many papers analyzing the kinematics and kinetics of the human knee, most have been cadaver studies that were controlled under artificial tension of muscles or ligaments. In these in vitro studies, various knee simulators were controlled by various mathematically derived inputs.^{5, 6, 7, 16, 17, 21, 23, 27, 33, 34} Therefore, those data had some limitations regarding how well they reflect knee motion in vivo. Even in vivo studies using noninvasive transducers fixed with straps or using skin markers, include errors caused by skin and soft tissue movement. Several in vivo methods have been used including the goniometric^{8, 9, 13, 14, 22, 24, 25, 29, 32} and photogrammetric^{1, 2, 3, 4, 12, 18, 26} methods. Thus, it is difficult to identify the more subtle movements of the knee joint, such as internal and external rotation and abduction and adduction. The knee motion is controlled by the function of the muscles in combination with geometric and ligamentous constraints. Consequently, there is still considerable question as to what constitutes normal motion at the knee in previous studies.

To overcome those issues, there have been studies in the literature that use invasive methods to precisely measure three-dimensional kinematics in the normal knee in vivo. In one study, knee motion was measured during gait by the photogrammetric method, using insertion of Steinmann traction pins into the femur and tibia, reported by Lafortune et al.¹⁵ In other studies, after insertion of 0.8 mm tantalum balls into the tibia and femur, they were tracked using stereophotogrammetry with radiographs, as reported by Kärrholm et al.^{10, 11} and Nilsson et al.^{19, 20} Although their amount of rotations and translations were not completely coincident with this present study because of different muscle condition during measurement (one was knee motion during gait and the others were that of prone position), intersubjective difference, and use of different coordinate systems, most patterns were in agreement to the present study (Fig 4).

The authors' method of in vivo insertion of K wires into the femur and tibia of human subjects, as was done in this study, is also highly invasive, however, it has several advantages. It allowed the authors to obtain serial knee kinematics during active flexion and extension in a sitting position as contrasted with the quasistatic procedure using stereophotogrammetry with radiographs. If the electrogoniometers are applied to the cadaver in the same manner as this study, it will enable researchers to simulate normal knee kinematics in a cadaver study. Furthermore, because this system can be fixed to a patient's leg with straps, which are noninvasive and easy to apply in clinical use, the effect of movement of superimposed soft tissues may be accounted for, knowing the discrepancy between the two types of fixation. This study provided an accurate description of knee kinematics in vivo without superimposed soft tissue motion. If the cadaver studies with knee simulator or testing

device used these data as input, researchers might obtain much more physiologic and significant data than the present.

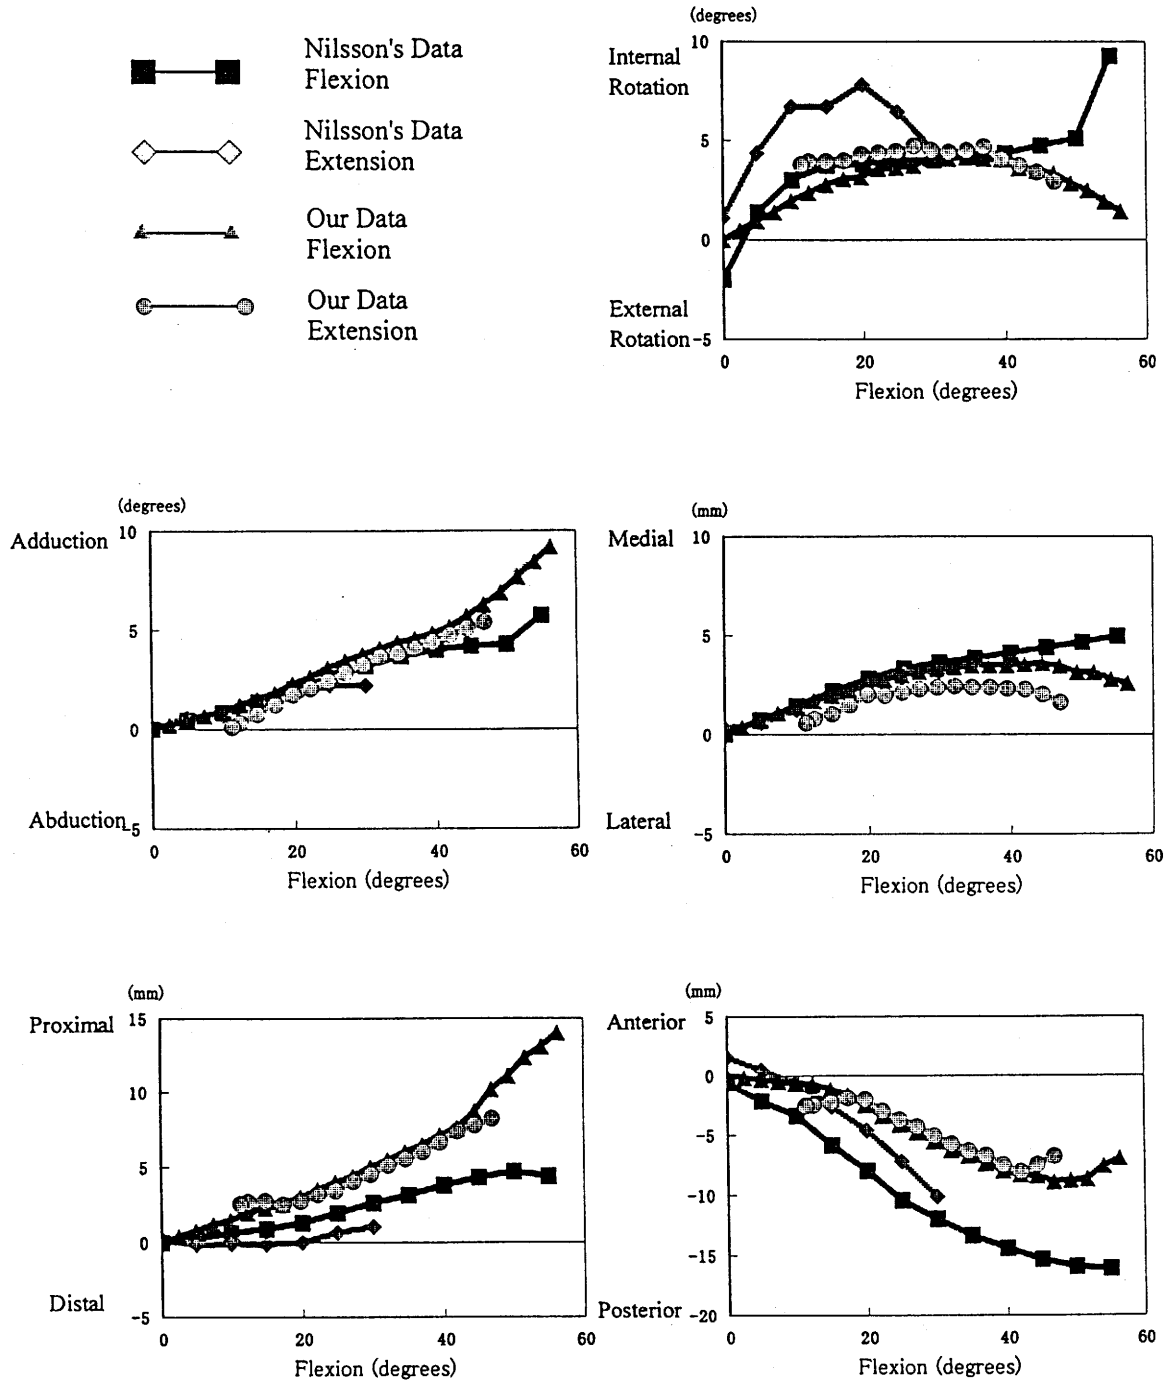


Figure 4: The data were translated by the coordinate system of Nilsson et al.²⁰ Most patterns were in agreement with those seen in the present study.

5. CONCLUSION

This study provided an accurate description of knee kinematics in vivo without superimposed soft tissue motion.

Acknowledgements.

The authors special thank Yoshinori Ishii MD, Department of Orthopaedic Surgery, School of Medicine, Niigata Univ. for his corporations. The authors also thank Joan E. Bechtold PhD, Director, Biomechanics Laboratory, Hennepin County Medical Center, Minneapolis, MN, for her assistance with the manuscript.

REFERENCES

1. Andriacchi TP, Andersson GB, Fermire RW, Stern D, Galante JO ; A study of lower-limb mechanics during stair-climbing, *J Bone Joint Surg* 62A: 749-757, 1980.
2. Andriacchi TP, Galante JO, Fermire RW ; The influence of total knee-replacement design on walking and stair-climbing, *J Bone Joint Surg* 64A : 1328-1335, 1982.
3. Berchuck M, Andriacchi TP ; Gait adaptations by patients who have a deficient anterior cruciate ligament, *J Bone Joint Surg* 72A : 871-877, 1990.
4. Goh JCH, Bose K, Khoo BCC ; Gait analysis study on patients with varus osteoarthritis of the knee, *Clin Orthop* 294 : 223-231, 1993.
5. Granberry WM, Noble PC, Woods GW ; Evaluation of an electrogoniometric instrument for measurement of laxity of the knee, *J Bone Joint Surg* 72A : 1316-1322, 1990.
6. Grood ES, Stowers SF, Noyes FR ; Limits of movement in human knee : Effect of sectioning the posterior cruciate ligament and posterolateral structures, *J Bone Joint Surg* 70A : 88-97, 1988.
7. Heegaard J, Leyvraz P-F, Kampen AV, et al ; Influence of soft structures on patellar three-dimensional tracking, *Clin Orthop* 299 : 235-243, 1994.
8. Ishii Y, Terajima K, Bechtold JE, Gustilo RB ; Effect of muscle force and posterior cruciate ligament retention on screw home motion after total knee replacement, *Trans Orthop Res Soc* 19 : 429, 1994.
9. Ishii Y, Terajima K, Gustilo RB; Comparison of knee joint laxity after total knee replacement with posterior cruciate retaining and substituting prosthesis, *Trans Orthop Res Soc* 18 : 429, 1993.
10. Kärrholm J ; Roentogen stereophotogrammetry : Review of orthopaedic applications, *Acta Orthop Scand* 60 : 491-503, 1989.
11. Kärrholm J, Selvic G, Elmqvist LG, Hansson LI ; Active knee motion after cruciate ligament rupture. Stereoradiography, *Acta Orthop Scand* 59 : 158-164, 1988.
12. Kelman GJ, Biden EN, Wyatt MP, Ritter MA, Colwell Jr CW ; Gait laboratory analysis of a posterior cruciate-sparing total knee arthroplasty in stair ascent and descent.

Clin Orthop 248 : 21-26, 1989.

13. Kettelkamp DB, Johnson RJ, Smidt GL, Chao EYS, Walker M ; An electrogoniometric study of knee motion in normal gait, J Bone Joint Surg 52A : 775-790, 1970.
14. Kinzel GL, Hall AS, Hillberry BM; Measurement of the total knee motion between two body segments : I. Analytic development, J Biomech 5 : 93-105, 1972.
15. Lafortune MA, Cavanagh PR, Sommer III HJ, Kalenak A ; Three-dimensional kinematics of the human knee during walking, J Biomech 25 : 347-357, 1992.
16. Markolf KL, Barger WL, Schoemaker SC, Amstutz HC ; The role of the joint load in knee stability. J Bone Joint Surg 63A : 570-585, 1981.
17. Mclain RF, Bargar WF; The effect of total knee design on patellar strain, J Arthroplasty 1 : 91-98, 1986.
18. Murray MP, Drought AB, Kory RC ; Walking pattern of normal men. J Bone Joint Surg 46A : 335-360, 1964.
19. Nilsson KG, Kärrholm J, Ekelund L ; Knee motion in total knee arthroplasty : A roentgen stereophotogrammetric analysis of the kinematics of the Tricon M knee prosthesis, Clin Orthop 256 : 147-161, 1990.
20. Nilsson KG, Kärrholm J, Gadegaard P ; Abnormal kinematics of the artificial knee. Roentgen stereophotometric analysis of 10 Miller-Galante and five New Jersey LCS knees. Acta Orthop Scand 62 : 440-446, 1991.
21. Petersilge WJ, Oishi CS, Kaufman KR, Irby SE, Colwell Jr CW ; The effect of trochlear design on patellofemoral shear and compressive forces in total knee arthroplasty, Clin Orthop 309 : 124-130, 1994.
22. Rittman N, Kettelkamp DB, Pryor P, Schwartzkopfe GL, Hillberry B ; Analysis of patterns of knee motion walking for four types of total knee implants, Clin Orthop 155: 111-117, 1981.
23. Sapega AA, Moyer RA, Schneck C, Komalahiranya N ; Testing for isometry during reconstruction of the anterior cruciate ligament : Anatomical and biomechanical considerations, J Bone Joint Surg 72A : 259-267, 1990.
24. Shiavi R, Limbird T, Frazer M, et al ; Helical motion analysis of the knee-I : Methodology for studying kinematics during locomotion, J Biomech 20 : 459-469, 1987.
25. Shiavi R, Limbird T, Frazer M, et al ; Helical motion analysis of the knee-II: Kinematics of uninjured and injured knees during walking and pivoting, J Biomech 20 ; 653-665, 1987.
26. Simmon SR, Trieshmann HW, Burdett RG, Ewald FC, Sledge CB : Quantitative gait analysis after total knee arthroplasty for monarticular degenerative arthritis, J Bone Joint Surg 65A : 605-613, 1983.
27. Skyhar MJ, Warren RF, Ortiz GJ, Schwartz E, Otis JC; The effects of sectioning of posterior cruciate ligament and the posterolateral complex on the articular

- contact pressure within the knee. J Bone Joint Surg 75A : 694-699, 1993.
28. Terajima K, Hara T, Koga Y, Nagata T ; Development of the three dimensional knee motion analysis system using computed radiography system, Proceedings of 1991 Annual meeting of Japanese Society for Orthopaedic Biomechanics, Sendai, Japan 13 : 213-217, 1991.
29. Terajima K, Ishii Y, Gustilo RB; Comparison of three-dimensional kinematics of total knee replacements with and without posterior cruciate ligament retention, Trans Orthop Res Soc 18 : 430, 1993.
30. Terajima K, Terashima S, Hara T, Ishii Y, Koga Y ; Definition of Three-Dimensional Motion Parameters for the Analysis of Knee Joint Motion, In Hirasawa Y, Sledge CB, Woo SL-Y, (eds), Clinical Biomechanics and Related Research. Tokyo, Springer-Verlag 383-391, 1994.
31. Terajima K, Tsuchiya Y, Hara T, Ishii T, Koga Y: Reliability evaluation of three dimensional knee motion analysis using computed radiography system, Proceedings of 1991 Annual meeting of Japanese Society for Orthopaedic Biomechanics, Sendai, Japan 13; 219-223, 1991.
32. Townsend MA, Izak M, Jackson RW: Total motion knee goniometry. J Biomech 10 ; 183-193, 1977.
33. Werner F, Mech M, Foster D, Murray DG ; The influence of design on transmission of torque across knee prostheses. J Bone Joint Surg 60A ; 342-348, 1978.
34. Whiteside LA, Kasselt MR, Haynes DW ; Varus-valgus and rotational stability in rotationally unconstrained total knee arthroplasty. Clin Orthop 219: 147-157, 1987.